Digital universal partical concentration sensor

PMSA003 series data manual

Writer	Zhou Yong	Version	V2.6
Verifier	Zheng Haoxin	Data	2018-02-26

Main characteristics

- ◆ Zero false alarm rate
- Real-time response
- ◆ Correct data
- Minimum distinguishable particle diameter :0.3 micrometer
- ◆ High anti-interference performance because of the patent structure of six sides shielding
- Optional direction of air inlet and outlet in order to adapt the different design
- ♦ Smallest

Overview

PMSA003I is a kind of digital and universal particle concentration sensor, which can be used to obtain the number of suspended particles in the air, i.e. the concentration of particles, and output them in the form of digital interface. This sensor can be inserted into variable instruments related to the concentration of suspended particles in the air or other environmental improvement equipments to provide correct concentration data in time.



Working principle

Laser scattering principle is used for such sensor, i.e. produce scattering by using laser to radiate suspending particles in the air, then collect scattering light in a certain degree, and finally obtain the curve of scattering light change with time. In the end, equivalent particle diameter and the number of particles with different diameter per unit volume can be calculated by microprocessor based on MIE theory. Please find the functional diagram of each part of sensor from Figure 1 as follows.

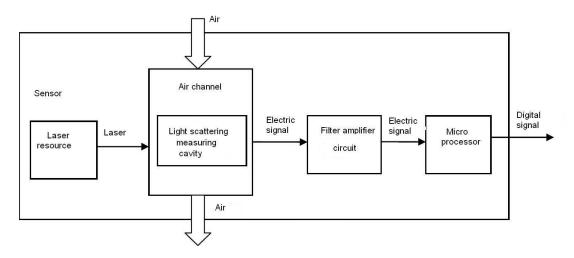


Figure 1 Functional block diagram of sensor

Technical Index


Parameter	Index	unit
Particle Range of measurement	0.3~1.0; 1.0~2.5; 2.5~10	Micrometer (μ m)
Particle Counting Efficiency	50%@0.3 μ m 98%@>=0.5 μ m	
Particle Effective Range (PM2.5	0~500	μg/m³
standard)		
Particle Maximum Range	≥1000	μ g/m³
(PM2.5 standard) *		
Particle Resolution	1	μg/m³
Particle Maximum Consistency	±10%@100~500 μ g/m³	
Error (PM2.5 standard data)*	\pm 10 μ g/m³ @0~100 μ g/m³	

Particle Standard Volume	0.1	Litre (L)
Single Response Time	<1	Second (s)
Total Response Time	≤10	Second (s)
DC Power Supply	Typ:5.0 Min:4.5 Max: 5.5	Volt (V)
Active Current	≤100	Milliampere (mA)
Standby Current	≤200	Microampere (μA)
Interface Level	L <0.8 @3.3 H >2.7@3.3	Volt (V)
Working Temperature Range	-10~+60	°C
Working Humidity Range	0~99%	
Storage Temperature Range	-40~+80	$^{\circ}$
MTTF	≥3	Year (Y)
Physical Size	38 ×35×12	Millimeter (mm)

Note 1: Maximum range means that the highest output value of the PM2.5 standard data is not less than 1000.

Note 2: "PM2.5 standard data" is the "data2" in the appendix.

Pin Definition



引脚定义:
Pin1-------VCC
Pin2------GND
Pin4-------GND
Pin5--------Reset
Pin6-------N/C
Pin7-------RXD
Pin8-------N/C
Pin9-------TXD
Pin10-------Set

Figure 2 Connector Definition

Pin number	Pin name	Description		
PIN1	VCC	Positive power 5V		
PIN2	VCC	Positive power 5V		
PIN3	GND	Negative power		
PIN4	GND	Negative power		
PIN5	RESET	Module reset signal/TTL level@3.3V, low reset		
PIN6	NC			
PIN7	RXD	Serial port receiving pin /TTL level@3.3V		
PIN8	NC			
PIN9	SDA	Serial port sending pin/TTL level@3.3V		
PIN10	SET	Set pin/TTL level @3.3V, high level or		
		suspending is normal working status, while low		
		level is sleeping mode.		

Output result

Mainly output as the quality and number of each particles with different size per unit volume, the unit volume of particle number is 0.1L and the unit of mass concentration is $\mu g/m^3$.

There are two options for digital output: passive and active. Default mode is active after power up. In this mode sensor would send serial data to the host automatically. The active mode is divided into two sub-modes:stable mode and fast mode. If the concentration change is small the sensor would run at stable mode with the real interval of 2.3s.And if the change is big the sensor would be changed to fast mode automatically with the interval of 200~800ms, the higher of the concentration, the shorter of the interval.

Typical Circuit

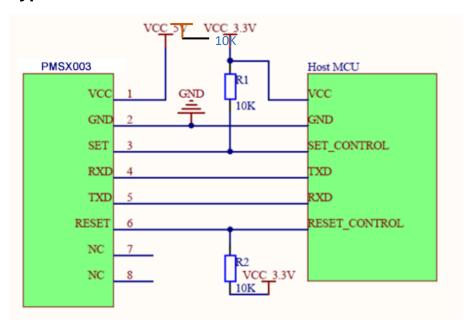


Figure 3 Typical Circuit

Typical Output Characteristic

Definition of axis Y: PM2.5 concentration, unit: µg/m³ Definition of axis X: number of samples, unit: time

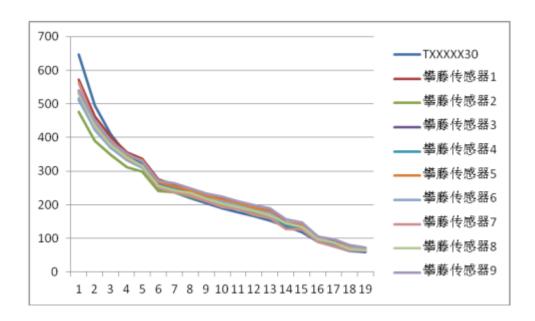


Figure 4-1 Consistency at 20℃

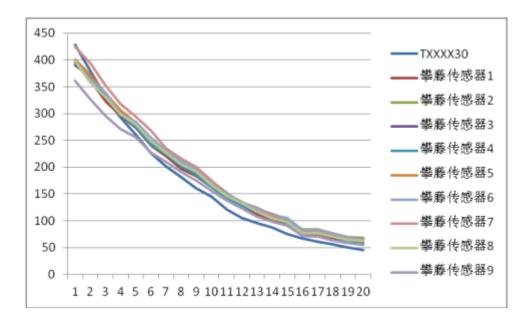


Figure 4-2 Consistency at 43°C

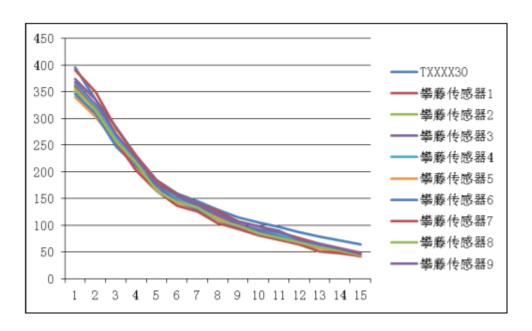


Figure 4-3 Consistency at -5°C

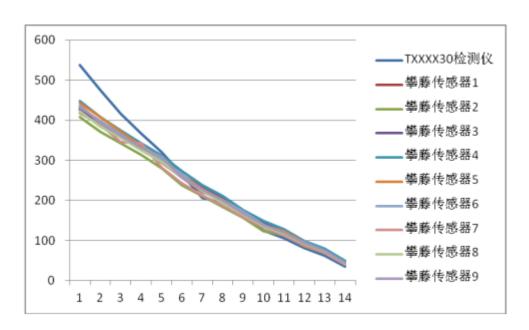


Figure 4-4 Consistency after 30 days running

Relationship of Temperature and Consistency

Definition of axis Y: Maximum Error Modulus(%)

Definition of axis X: Temperature(°C)

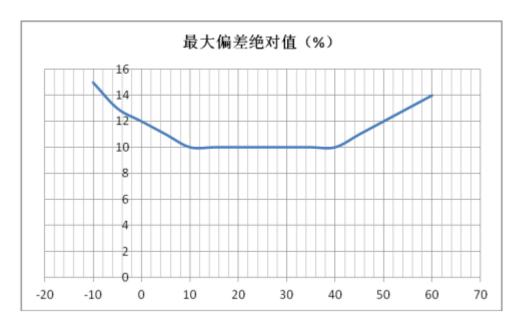


Figure 5 Consistency Vs Temperature

Endurance Characteristics

No	Item	Tes	t Method	Characteristics	n
				0.10.10000100100	С
1	Long Running	1	10 m² closed Lab, 20~25°C,	10 samples during	n=30
-	Long Kaming	1.	humidity 30%~70%, particle	0~500 μ g/m ³	C=0
			generator and air cleaner	0 300 F g/III	C-0
		2	•	00400 11 0 /m3	
		2.	DC 5V power supply	0~100 μ g/m³	
		3.	Check consistency after 720	Maximum Error ≤	
			hours' running	\pm 15 μ g/m 3	
2	High	1.	10 m² constant temperature Lab		n=10
	Temperature	2.	43℃,humidity 70%,	100~500 μ g/m ³	C=0
	Operation	3.	particle generator and air	Maximum Error ≤	
			cleaner	\pm 15%	
		4.	DC 5V power supply		
		5.	Check consistency		
3	Cold Operation	1.	10 m² constant temperature Lab	FAN does not	n=10
		2.	-5℃,humidity 30%,	screeched	C=0
		3.	particle generator and air		
			cleaner		
		4.	DC 5V power supply		
		5.	Check consistency		

4	Vibration	1.	10 M^2 closed Lab, 20°C ,		n=5
			humidity 50%, particle		C=0
			generator and air cleaner		
		2.	DC 5V power supply and check		
		_	consistency		
		3.	Frequency: 50Hz		
		4.	acceleration: 9.8/S ² o		
		5.			
		6.	Vibration Amplitude: ± 2 mm $_{\circ}$		
		7.	Time: X、Y、Z—way, Per 1 hour		
5	High	1.	Constant temperature cabinet	10 samples during	n=10
	Temperature	2.	70 $^{\circ}$ C ,humidity 90% $^{\sim}$ 95,	0~500 μ g/m³	C=0
	and Humidity	3.	Check consistency after 500		
	Storage	hou	urs' storage	0~100 μ g/m³	
				Maximum Error ≤	
6	Cold Storage	1.	Constant temperature cabinet	\pm 10 μ g/m 3	n=10
		2.	-30 $^{\circ}$ C ,humidity 90% $^{\sim}$ 95,		C=0
		3.	Check consistency after 500	100~500 µ g/m³	
		hou	urs' storage	Maximum Error ≤	
				±10%	
7	Variation of	4.	10 M^2 closed Lab, , 20 $^{\circ}\text{C}$,		n=5
	Power Supply		humidity 50%, particle		C=0
			generator and air cleaner	FAN does not	
				screeched	
		5.	Power varies as the cycles of 4.5V		
			to 5.5V ,then 5.5V to 4.5V with the		
			pace of 0.1V/min for 2 hours.		
		6.	Check consistency during		
			Variation		
8	Power On-Off	1.	10 $\mbox{ m}^{2}$ closed Lab, , 20 $^{\circ}\mbox{C}$,		n=10
	Cycle		humidity 50%, particle		C=0
			generator and air cleaner		
		2.	DC 5V power supply, keep On-		
			Off frequency 0.5Hz for 72 hours		
			and check consistency		
9	Sleep Set On-	1.	10 m² closed Lab, 20℃,		n=10
	Off		humidity 50%, particle		C=0
	Cycle		generator and air cleaner		
		2.	DC 5V power supply, keep Sleep		
			Set Pin High-Low frequency 0.5Hz		
			for 72 hours and check		
			consistency		
10	Laser On-Off	1.	10 m² closed Lab, 20 ℃ ,		n=10
	1			l .	

	Cycle	humidity 50%, particle		C=0
		generator and air cleaner		
		2. keep laser On-Off frequency		
		50Hz for 240 hours and check		
		consistency		
11	Salt Spray	5% industrial salt water, hydrolysis	No rust and	n=1
		spray 100 hours, clean with purified	discoloration of	C=0
		water and store for 48 hours	metal parts	

Circuit Attentions

- DC 5V power supply is needed because the FAN should be driven by 5V. But the high level of data pin is 3.3V. Level conversion unit should be used if the power of host MCU is 5V.
- 2) The SET and RESET pins are pulled up inside so they should not be connected if without usage.
- 3) PIN6 and PIN8 should not be connected.
- 4) Stable data should be got at least 30 seconds after the sensor wakeup from the sleep mode because of the fan's performance.


Installation Attentions

- 1) Metal shell is connected to the GND so be careful not to let it shorted with the other parts of circuit except GND.
- The best way of install is making the plane of inlet and outlet closely to the plane of the host. Or some shield should be placed between inlet and outlet in order to prevent the air flow from inner loop.
- 3) The blowhole in the shell of the host should not be smaller than the inlet.
- 4) The sensor should not be installed in the air flow way of the air cleaner or should be shielded by some structure.
- 5) The sensor should be installed at least 20cm higher than the grand in order to prevent it from blocking by the flock dust.
- 6) When the sensor is used to outdoor fixed equipment, the equipment should be completed for the protection of sandstorm,rain,snow,etc.
- 7) Do not break up the sensor.
- 8) The two screw holes can be used for positioning and fixing, For fixing holes, the screw depth can reach 3.4mm, and the other shoule not exceed 1.9mm.


Other Attentions

- Only the consistency of all the PM sensors of PLANTOWER is promised and ensured. And the sensor should not be checked with any third party equipment.
- 2) The sensor is usually used in the common indoor environment. So some protection must be added if using in the conditions as followed:
 - a) The time of concentration \geqslant 300 μ g/m³ is longer than 50% of the whole year or concentration \geqslant 500 μ g/m³ is longer than 20% of the whole year.
 - b) Kitchen
 - c) Water mist condition such as bathroom or hot spring.
 - d) Outdoor

Part Number Definition

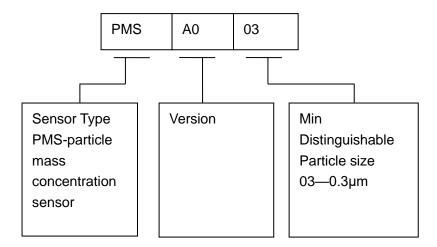

Physical Size(mm)

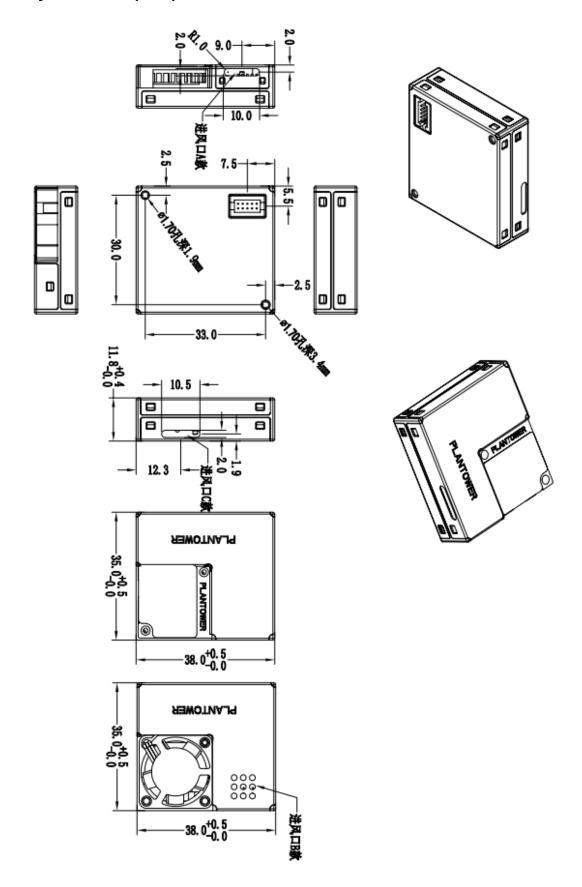

Appendix I: transport protocol-Active Mode

Default baud rate: 9600bps Check bit: None Stop bit: 1 bit

32 Bytes

0x42 (Fixed)		
0x4d	(Fixed)	
	Frame length=2x13+2(data+check bytes)	
	Data1 refers to PM1.0 concentration unit μ g/m3 (CF=1, standard particle) *	
	g/me (et 1) etamadia partiele/	
	Data2 refers to PM2.5 concentration unit μ g/m3 (CF=1, standard particle)	
	g/me (et 1) etamadia partiele/	
	Data3 refers to PM10 concentration unit μ g/m3 (CF=1, standard particle)	
	g/me (et =1) diamata particle)	
	Data4 refers to PM1.0 concentration unit * µ g/m3 (under atmospheric	
	environment)	
	Data 5 refers to PM2.5 concentration unit µ g/m3 (under atmospheric	
	environment)	
	Data 6 refers to concentration unit (under	
	atmospheric environment) µ g/m3	
	Data7 indicates the number of	
	particles with diameter beyond 0.3 um in 0.1 L of air.	
	Data 8 indicates the number of	
	particles with diameter beyond 0.5 um in 0.1 L of air.	
	Data 9 indicates the number of particles with diameter beyond 1.0	
	um in 0.1 L of air.	
	Data10 indicates the number of particles with diameter beyond 2.5	
	um in 0.1 L of air.	
	0x4d	

Data11 high 8 bits	 Data11 indicates the number of particles with diameter beyond 5.0
Data11 low 8 bits	 um in 0.1 L of air.
Data12 high 8 bits	 Data12 indicates the number of particles with diameter beyond 10 um
Data12 low 8 bits	 in 0.1 L of air.
Data13 high 8 bits	 Version
Data13 low 8 bits	 error code
Data and check high 8 bits	 Check code=Start character 1+ Start character 2++data 13
Data and check low 8 bits	 Low 8 bits

Note: CF=1 should be used in the factory environment

.

Appendix II: transport protocol-Passive Mode

Default baud rate: 9600bps Check bit: None Stop bit: 1 bit

Host Protocol

Start Byte	Start Byte	Command	Data 1	Data 2	Verify	Verify
1	2				Byte 1	Byte 2
0x42	0x4d	CMD	DATAH	DATAL	LRCH	LRCL

1. Command Definition

CMD	DATAH	DATAL	Note
0xe2	X	X	Read in passive
			mode
0xe1	X	00H-passive	Change mode
		01H-active	
0xe4	Х	00H-sleep	Sleep set
		01H-wakeup	

2. Answer

0xe2: 32bytes , same as appendix I

3. Verify Bytes:

Add of all the bytes except verify bytes.